

Instructional Quick Guide for FOLLISTIM[®] AQ Cartridge (follitropin beta injection)

Directions provided here are abbreviated. They should be used only after receiving complete instructions from your health care professional.

To give yourself the injection, you will need:

- A FOLLISTIM AQ Cartridge, FOLLISTIM Pen[®], and a new BD Micro-Fine[™] Pen Needle provided with the Cartridge.
- A clean, dry surface, alcohol and cotton balls, or alcohol pads, sterile gauze, anti-bacterial soap, and a puncture-proof container to discard used supplies.

The FOLLISTIM AQ Cartridge is only for use with the FOLLISTIM Pen. Read all instructions carefully before using your FOLLISTIM Pen with the FOLLISTIM AQ Cartridge. Failure to do so could result in an incorrect dose being given.



Not actual size.

1. READY ▶ Prepare your FOLLISTIM Pen



Figure 1A

- Pull the protective cap off the Pen Body (Figure 1A) and put it aside on a clean, dry surface.
- Unscrew the entire Pen Body from the Cartridge Holder.
- Place Pen Body and Cartridge Holder on a clean, dry surface.



Figure 1B

- Remove the FOLLISTIM AQ Cartridge from its package and clean the rubber inlay of the Cartridge with an alcohol pad.
- Insert the Cartridge into the Cartridge Holder (Figure 1B), metal rimmed cap end first.
- Screw Pen Body fully onto the Cartridge Holder containing the inserted Cartridge (Figure 1C), making sure there are no gaps.



Figure 1C

- Line up the arrow (▲) with the middle of the yellow alignment mark (■).
- Clean the open end of the Cartridge Holder with an alcohol pad. Peel off the protective paper seal from the BD Micro-Fine Pen Needle that is in its Outer Needle Shield. Attach a new BD Micro-Fine Pen Needle after you make sure there is a FOLLISTIM AQ Cartridge in the FOLLISTIM Pen. Push the end of the Cartridge Holder into the Outer Needle Shield. Screw tightly together (Figure 1D).



Figure 1D

- **Your FOLLISTIM Pen is now assembled and loaded.**
- **Never touch the needle and never place an open needle on any surface.**
- You must use a new BD Micro-Fine Pen Needle with each injection.

BD Micro-Fine Pen Needle is a trademark of Becton-Dickinson.

2. SET ► Set your dose



Figure 2A

- Use an alcohol pad to clean about a 2-inch area of skin where the needle will enter.
- Gently pull off the Outer Needle Shield, leaving the Inner Needle Shield in place (Figure 2A), and set aside. Do not discard the Outer Needle Shield.



Figure 2B

- Carefully remove the Inner Needle Shield (Figure 2B) and discard.
- Do not touch the needle or let it touch any surface while uncapped.
- Hold the FOLLISTIM Pen® with the needle pointing upwards. Tap the Cartridge Holder with your finger to force air bubbles to the top of the needle.
- Dial the Dosage Knob until you hear one click. With the needle pointing upwards, push in the Injection Button.
- Look for a droplet of medicine at the needle tip (Figure 2C). If you do not see a droplet, repeat steps above; otherwise you might not receive the correct dose.



Figure 2C

- If you have already used the FOLLISTIM® AQ Cartridge (follitropin beta injection) and you need to give yourself another dose, attach a new BD Micro-Fine™ Pen Needle and look for a droplet forming at the tip of the needle. If you do not see a droplet, repeat the previous 2 steps.



Figure 2D

- For doses of 50 International Units (IU) up to 450 IU, turn the Dosage Knob until the correct dosage aligns with the dosage markers on each side of the Dosage Window (Figure 2D).
- If you dial past your dose, do not turn the Dosage Knob backward (you will not damage the Pen, but medicine will be lost). Continue turning until you pass the 450 IU mark, as far as it will turn. The Dosage Knob must move freely.
- Push the Injection Button in as far as it will go. Start dialing from “0” upwards until you reach the correct dosage.
- You are now ready to complete your injection.
- Never try to correct a dose-dialing mistake while the needle is in your skin. This may result in an incorrect dose.
- If your prescribed dose exceeds the deliverable dose of the FOLLISTIM Pen or exceeds the amount remaining in the Cartridge, you will need to give yourself more than one injection.

3. INJECT ► Inject your FOLLISTIM AQ Cartridge



Figure 2E

- Pinch the cleansed skin area between 2 fingers. With your other hand, insert the entire Pen Needle straight into the skin at a 90-degree angle (Figure 2E). Press the Injection Button all the way. Wait 5 seconds. The middle of the Dosage Window should display a dot next to the “0”. Pull the needle out quickly and apply pressure to the injection site with an alcohol pad. Maintaining pressure, gently massage the site.
- The best places to inject are just below your belly button or the upper outer area of your thigh.
- If the number in the Dosage Window does not read “0” and you cannot push the Injection Button all the way in, do not try to force down the button. Your FOLLISTIM AQ Cartridge is probably empty. This means you have not received your full dose. Do not adjust the setting on the Dosage Scale. The number in the Dosage Window is the amount needed to complete your prescribed dose. Write down this number. Remove the needle and dispose of it properly. Reset the Dial Window to “0” by turning the Dosage Knob past the 450 IU mark as far as it will turn and pushing the injection button all the way in. Repeat instructions from “Ready (►) Prepare Your FOLLISTIM Pen to load a new Cartridge, attach a new needle and inject the remaining drug to complete your dose”.
- Your injection is complete!

Storage and Disposal

- Each Pen Needle is for one injection only. Immediately following injection, remove and dispose of the used Pen Needle. The Pen Needle must be removed from the FOLLISTIM Pen prior to storage.

Please read the accompanying Patient Information for FOLLISTIM AQ Cartridge and discuss it with your doctor. The physician Prescribing Information also is available.



HIGHLIGHTS OF PRESCRIBING INFORMATION

These highlights do not include all the information needed to use FOLLISTIM® AQ Cartridge safely and effectively. See full prescribing information for FOLLISTIM® AQ Cartridge.

FOLLISTIM® AQ Cartridge (follitropin beta injection) for subcutaneous use
Initial U.S. Approval: 1997

-----INDICATIONS AND USAGE-----
Follistim AQ Cartridge is a gonadotropin indicated:

In Women for:

- Induction of Ovulation and Pregnancy in Anovulatory Infertile Women in Whom the Cause of Infertility is Functional and Not Due to Primary Ovarian Failure (1.1)
- Pregnancy in Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization (IVF) or Intracytoplasmic Sperm Injection (ICSI) Cycle (1.2)

In Men for:

- Induction of Spermatogenesis in Men with Primary and Secondary Hypogonadotropic Hypogonadism (HH) in Whom the Cause of Infertility is Not Due to Primary Testicular Failure (1.3)

-----DOSAGE AND ADMINISTRATION-----
See Dose Conversion Table 1 for Follistim AQ Cartridge with Pen Injector (2.1)

In Anovulatory Women Undergoing Ovulation Induction (2.2):

- Starting daily dose of 50 international units of Follistim AQ Cartridge is administered subcutaneously for at least the first 7 days. The dose is increased by 25 or 50 international units at weekly intervals until follicular growth and/or serum estradiol levels indicate an adequate response.
 - When an acceptable pre-ovulatory state is achieved, final oocyte maturation is achieved with 5,000 to 10,000 international units of human chorionic gonadotropin (hCG).
 - The woman and her partner should have intercourse daily, beginning on the day prior to the administration of hCG and until ovulation becomes apparent.

In Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization or Intracytoplasmic Sperm Injection Cycle (2.3):

- Starting dose of 200 international units (actual cartridge doses) of Follistim AQ Cartridge is administered subcutaneously for at least the first 7 days of treatment. Subsequent doses can be adjusted down or up based upon ovarian response as determined by ultrasound evaluation of follicular growth and serum estradiol levels. Dosage reduction in high responders can be considered from the 6th day of treatment onward according to individual response.
 - Final oocyte maturation is induced with a dose of 5,000-10,000 international units of hCG.
 - Oocyte (egg) retrieval is performed 34 to 36 hours later.

Induction of Spermatogenesis in Men (2.4):

- Pretreatment with hCG alone (1,500 international units twice weekly) is required. If serum testosterone levels have not normalized after 8 weeks of hCG treatment, the dose may be increased to 3,000 international units twice a week.
- After normalization of serum testosterone levels, administer 450 international units per week (225 international units twice weekly or 150 international units three times weekly) of Follistim AQ

Cartridge subcutaneously with the same pre-treatment hCG dose used to normalize testosterone levels.

-----DOSAGE FORMS AND STRENGTHS-----

- Injection: Follistim AQ Cartridge 175 IU per 0.210 mL (3)
- Injection: Follistim AQ Cartridge 350 IU per 0.420 mL (3)
- Injection: Follistim AQ Cartridge 650 IU per 0.780 mL (3)
- Injection: Follistim AQ Cartridge 975 IU per 1.170 mL (3)

-----CONTRAINDICATIONS-----

Women and men who exhibit:

- Prior hypersensitivity to recombinant hFSH products (4)
- High levels of FSH indicating primary gonadal failure (4)
- Presence of uncontrolled non-gonadal endocrinopathies (4)
- Hypersensitivity reactions related to streptomycin or neomycin (4)
- Tumors of the ovary, breast, uterus, testis, hypothalamus or pituitary gland (4)

Women who exhibit:

- Pregnancy (4, 8.1)
- Heavy or irregular vaginal bleeding of undetermined origin (4)
- Ovarian cysts or enlargement not due to polycystic ovary syndrome (PCOS) (4)

-----WARNINGS AND PRECAUTIONS-----

Treatment with Follistim AQ may result in:

- Abnormal Ovarian Enlargement (5.1)
- Ovarian Hyperstimulation Syndrome (OHSS) (5.2)
- Pulmonary and Vascular Complications (5.3)
- Ovarian Torsion (5.4)
- Multi-fetal Gestation and Birth (5.5)
- Congenital Anomalies (5.6)
- Ectopic Pregnancy (5.7)
- Spontaneous Abortion (5.8)
- Ovarian Neoplasms (5.9)

-----ADVERSE REACTIONS-----

The most common adverse reactions (≥2%) in women undergoing ovulation induction are ovarian hyperstimulation syndrome, ovarian cyst, abdominal discomfort, abdominal pain and lower abdominal pain. (6.1)

The most common adverse reactions (≥2%) in women undergoing controlled ovarian stimulation as part of an IVF or ICSI cycle are pelvic discomfort, headache, ovarian hyperstimulation syndrome, pelvic pain, nausea and fatigue. (6.1)

The most common (≥2%) adverse reactions in men undergoing induction of spermatogenesis are headache, acne, injection site reaction, injection site pain, gynecomastia, rash and dermoid cyst. (6.1)

To report SUSPECTED ADVERSE REACTIONS, contact Merck Sharp & Dohme Corp., a subsidiary of Merck & Co., Inc., at 1-877-888-4231 or FDA at 1-800-FDA-1088 or www.fda.gov/medwatch.

-----USE IN SPECIFIC POPULATIONS-----

Nursing Mothers: It is not known whether this drug is excreted in human milk. (8.3)

See 17 for PATIENT COUNSELING INFORMATION and FDA-approved patient labeling.

Revised: 06/2020

FULL PRESCRIBING INFORMATION: CONTENTS***1 INDICATIONS AND USAGE**

- 1.1 Induction of Ovulation and Pregnancy in Anovulatory Infertile Women in Whom the Cause of Infertility is Functional and Not Due to Primary Ovarian Failure
- 1.2 Pregnancy in Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization (IVF) or Intracytoplasmic Sperm Injection (ICSI) Cycle
- 1.3 Induction of Spermatogenesis in Men with Primary and Secondary Hypogonadotropic Hypogonadism (HH) in Whom the Cause of Infertility is Not Due to Primary Testicular Failure

2 DOSAGE AND ADMINISTRATION

- 2.1 General Dosing Information
- 2.2 Recommended Dosing in Anovulatory Women Undergoing Ovulation Induction
- 2.3 Recommended Dosing in Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization (IVF) or Intracytoplasmic Sperm Injection (ICSI) Cycle
- 2.4 Recommended Dosing for Induction of Spermatogenesis in Men

3 DOSAGE FORMS AND STRENGTHS**4 CONTRAINDICATIONS****5 WARNINGS AND PRECAUTIONS**

- 5.1 Abnormal Ovarian Enlargement
- 5.2 Ovarian Hyperstimulation Syndrome (OHSS)
- 5.3 Pulmonary and Vascular Complications
- 5.4 Ovarian Torsion
- 5.5 Multi-fetal Gestation and Birth
- 5.6 Congenital Anomalies
- 5.7 Ectopic Pregnancy
- 5.8 Spontaneous Abortion
- 5.9 Ovarian Neoplasms

5.10 Laboratory Tests

5.11 Follistim Pen

6 ADVERSE REACTIONS

- 6.1 Clinical Study Experience
- 6.2 Postmarketing Experience

7 DRUG INTERACTIONS**8 USE IN SPECIFIC POPULATIONS**

- 8.1 Pregnancy
- 8.3 Nursing Mothers
- 8.4 Pediatric Use
- 8.5 Geriatric Use

10 OVERDOSAGE**11 DESCRIPTION****12 CLINICAL PHARMACOLOGY**

- 12.1 Mechanism of Action
- 12.3 Pharmacokinetics

13 NONCLINICAL TOXICOLOGY

- 13.1 Carcinogenesis, Mutagenesis, Impairment of Fertility

14 CLINICAL STUDIES

- 14.1 Ovulation Induction
- 14.2 Controlled Ovarian Stimulation as Part of an In Vitro Fertilization (IVF) or Intracytoplasmic Sperm Injection (ICSI) Cycle
- 14.3 Induction of Spermatogenesis

16 HOW SUPPLIED/STORAGE AND HANDLING**17 PATIENT COUNSELING INFORMATION**

- 17.1 Dosing and Use of Follistim AQ Cartridge with Pen
- 17.2 Therapy Duration and Necessary Monitoring in Women and Men Undergoing Treatment
- 17.3 Instructions on a Missed Dose
- 17.4 Ovarian Hyperstimulation Syndrome
- 17.5 Multi-fetal Gestation and Birth

* Sections or subsections omitted from the full prescribing information are not listed.

FULL PRESCRIBING INFORMATION

1 INDICATIONS AND USAGE

Follistim® AQ (follitropin beta injection) Cartridge is indicated:

In Women for:

1.1 Induction of Ovulation and Pregnancy in Anovulatory Infertile Women in Whom the Cause of Infertility is Functional and Not Due to Primary Ovarian Failure

Prior to initiation of treatment with Follistim AQ Cartridge:

- Women should have a complete gynecologic and endocrinologic evaluation.
- Primary ovarian failure should be excluded.
- The possibility of pregnancy should be excluded.
- Tubal patency should be demonstrated.
- The fertility status of the male partner should be evaluated.

1.2 Pregnancy in Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization (IVF) or Intracytoplasmic Sperm Injection (ICSI) Cycle

Prior to initiation of treatment with Follistim AQ Cartridge:

- Women should have a complete gynecologic and endocrinologic evaluation and diagnosis of cause of infertility.
- The possibility of pregnancy should be excluded.
- The fertility status of the male partner should be evaluated.

In Men for:

1.3 Induction of Spermatogenesis in Men with Primary and Secondary Hypogonadotropic Hypogonadism (HH) in Whom the Cause of Infertility is Not Due to Primary Testicular Failure

Prior to initiation of treatment with Follistim AQ Cartridge:

- Men should have a complete medical and endocrinologic evaluation.
- Hypogonadotropic hypogonadism should be confirmed and primary testicular failure should be excluded.
- Serum testosterone levels should be normalized with human chorionic gonadotropin (hCG) treatment.
- The fertility status of the female partner should be evaluated.

2 DOSAGE AND ADMINISTRATION

2.1 General Dosing Information

- Parenteral drug products should be inspected visually for particulate matter and discoloration prior to administration, whenever solution and container permit. If the solution is not clear and colorless or has particles in it, the solution should not be used.
- Do not add any other medicines into the Follistim AQ Cartridge.
- Follistim AQ Cartridge with the pen injector device delivers on average an 18% higher amount of follitropin beta when compared to reconstituted Follistim delivered with a conventional syringe and needle. When administering Follistim AQ Cartridge, a lower starting dose and lower dose adjustments (as compared to reconstituted Follistim) should be considered. For that purpose the following Dose Conversion Table is provided:

Table 1: Follistim AQ Cartridge Administered Subcutaneously With the Follistim Pen Dose Conversion Table*

Lyophilized recombinant FSH dosing with ampules or vials, using conventional syringe	Follistim AQ Cartridge dosing with the Follistim Pen
75 IU	50 IU
150 IU	125 IU
225 IU	175 IU
300 IU	250 IU
375 IU	300 IU
450 IU	375 IU

* Each value represents an 18% difference rounded to the nearest 25 IU increment.

2.2 Recommended Dosing in Anovulatory Women Undergoing Ovulation Induction

The dosing scheme is stepwise and is individualized for each woman [see *Clinical Studies (14.1)*].

- A starting daily dose of 50 international units of Follistim AQ Cartridge is administered [see *Dosage and Administration (2.1)*] subcutaneously daily for at least the first 7 days.
- Subsequent dosage adjustments are made at weekly intervals based upon ovarian response. If an increase in dose is indicated by the ovarian response, the increase should be made by 25 or 50 international units of Follistim AQ Cartridge at weekly intervals until follicular growth and/or serum estradiol levels indicate an adequate ovarian response.
The following should be considered when planning the woman's individualized dose:
 - Appropriate Follistim AQ Cartridge dose adjustment(s) should be used to prevent multiple follicular growth and cycle cancellation.
 - The maximum, individualized, daily dose of Follistim AQ Cartridge is 250 international units.
- Treatment should continue until ultrasonic visualizations and/or serum estradiol determinations approximate the pre-ovulatory conditions seen in normal individuals.
- When pre-ovulatory conditions are reached, 5,000 to 10,000 international units of hCG are used to induce final oocyte maturation and ovulation.

The administration of hCG must be withheld in cases where the ovarian monitoring suggests an increased risk of OHSS on the last day of Follistim AQ Cartridge therapy [see *Warnings and Precautions (5.1, 5.2, 5.10)*].

- The woman and her partner should be encouraged to have intercourse daily, beginning on the day prior to the administration of hCG and until ovulation becomes apparent [see *Warnings and Precautions (5.10)*].
- During treatment with Follistim AQ Cartridge and during a two-week post-treatment period, the woman should be assessed at least every other day for signs of excessive ovarian stimulation.

It is recommended that Follistim AQ Cartridge administration be stopped if the ovarian monitoring suggests an increased risk of OHSS or abdominal pain occurs. Most OHSS occurs after treatment has been discontinued and reaches its maximum at about seven to ten days post-ovulation.

2.3 Recommended Dosing in Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization (IVF) or Intracytoplasmic Sperm Injection (ICSI) Cycle

The dosing scheme follows a stepwise approach and is individualized for each woman.

- A starting dose of 200 international units (actual cartridge doses) of Follistim AQ Cartridge is administered [see *Dosage and Administration (2.1)*] subcutaneously daily for at least the first 7 days of treatment.
- Subsequent to the first 7 days of treatment, the dose can be adjusted down or up based upon the woman's ovarian response as determined by ultrasound evaluation of follicular growth and serum estradiol levels. Dosage reduction in high responders can be considered from the 6th day of treatment onward according to individual response.

The following should be considered when planning the woman's individualized dose:

- For most normal responding women, the daily starting dose can be continued until pre-ovulatory conditions are achieved (seven to twelve days).
- For low or poor responding women, the daily dose should be increased according to the ovarian response. The maximum, individualized, daily dose of Follistim AQ Cartridge is 500 international units.
- For high responding women [those at particular risk of abnormal ovarian enlargement and/or ovarian hyperstimulation syndrome (OHSS)], decrease or temporarily stop the daily dose, or discontinue the cycle according to individual response [see *Warnings and Precautions (5.1, 5.2, 5.10)*].
- When a sufficient number of follicles of adequate size are present, dosing of Follistim AQ Cartridge is stopped and final maturation of the oocytes is induced by administering hCG at a dose of 5,000 to 10,000 international units. The administration of hCG should be withheld in cases where the ovarian monitoring suggests an increased risk of OHSS on the last day of Follistim AQ Cartridge therapy [see *Warnings and Precautions (5.1, 5.2, 5.10)*].
- Oocyte (egg) retrieval should be performed 34 to 36 hours following the administration of hCG.

2.4 Recommended Dosing for Induction of Spermatogenesis in Men

- Pretreatment with hCG is required prior to concomitant therapy with Follistim AQ Cartridge and hCG. An initial dosage of 1,500 international units of hCG should be administered at twice weekly intervals to normalize serum testosterone levels. If serum testosterone levels have not normalized after 8 weeks of hCG treatment, the hCG dose can be increased to 3,000 international units twice weekly [see *Clinical Studies (14.3)*].
- After normal serum testosterone levels have been reached, Follistim AQ Cartridge should be administered by subcutaneous injection concomitantly with hCG treatment. Follistim is given at a dosage of 450 international units per week, as either 225 international units twice weekly or 150 international units three times per week, in combination with the same hCG dose used to normalize testosterone levels. Based on delivery of a higher dose of follitropin beta with the Follistim AQ Cartridge and pen injector [see *Dosage and Administration (2.1)*], a lower dose of Follistim AQ Cartridge may be considered.

The concomitant therapy should be continued for at least 3 to 4 months before any improvement in spermatogenesis can be expected. If a man has not responded after this period, the combination therapy may be continued. Treatment response has been noted at up to 12 months.

3 DOSAGE FORMS AND STRENGTHS

Injection: Follistim AQ Cartridge 175 international units per 0.210 mL

Injection: Follistim AQ Cartridge 350 international units per 0.420 mL

Injection: Follistim AQ Cartridge 650 international units per 0.780 mL

Injection: Follistim AQ Cartridge 975 international units per 1.170 mL

4 CONTRAINDICATIONS

Follistim AQ Cartridge is contraindicated in women and men who exhibit:

- Prior hypersensitivity to recombinant hFSH products
- High levels of FSH indicating primary gonadal failure
- Presence of uncontrolled non-gonadal endocrinopathies (e.g., thyroid, adrenal, or pituitary disorders) [see *Indications and Usage (1.1, 1.2, 1.3)*]
- Hypersensitivity reactions to streptomycin or neomycin. Follistim AQ may contain traces of these antibiotics
- Tumors of the ovary, breast, uterus, testis, hypothalamus or pituitary gland

Follistim AQ Cartridge is also contraindicated in women who exhibit:

- Pregnancy [see *Use in Specific Populations (8.1)*]
- Heavy or irregular vaginal bleeding of undetermined origin
- Ovarian cysts or enlargement not due to polycystic ovary syndrome (PCOS)

5 WARNINGS AND PRECAUTIONS

Follistim AQ Cartridge should be used only by physicians who are experienced in infertility treatment. Follistim AQ Cartridge contains a potent gonadotropic substance capable of causing Ovarian Hyperstimulation Syndrome (OHSS) [see *Warnings and Precautions (5.2)*] with or without pulmonary or vascular complications [see *Warnings and Precautions (5.3)*] and multiple births [see *Warnings and Precautions (5.5)*]. Gonadotropin therapy requires the availability of appropriate monitoring facilities [see *Warnings and Precautions (5.10)*].

Careful attention should be given to the diagnosis of infertility and in the selection of candidates for Follistim AQ Cartridge therapy [see *Indications and Usage (1.1, 1.2, 1.3) and Dosage and Administration (2.2, 2.3, 2.4)*].

Switching to Follistim AQ Cartridge from other brands (manufacturer), types (recombinant, urinary), and/or methods of administration (Follistim Pen, conventional syringe) may necessitate an adjustment of the dose [see *Dosage and Administration (2)*].

5.1 Abnormal Ovarian Enlargement

In order to minimize the hazards associated with abnormal ovarian enlargement that may occur with Follistim AQ therapy, treatment should be individualized and the lowest effective dose should be used [see *Dosage and Administration (2.2, 2.3)*]. Use of ultrasound monitoring of ovarian response and/or measurement of serum estradiol levels is important to minimize the risk of overstimulation [see *Warnings and Precautions (5.8)*].

If the ovaries are abnormally enlarged on the last day of Follistim AQ therapy, hCG should not be administered in order to reduce the chances of developing Ovarian Hyperstimulation Syndrome (OHSS). Intercourse should be prohibited in patients with significant ovarian enlargement after ovulation because of the danger of hemoperitoneum resulting from ruptured ovarian cysts [see *Warnings and Precautions (5.3)*].

5.2 Ovarian Hyperstimulation Syndrome (OHSS)

OHSS is a medical entity distinct from uncomplicated ovarian enlargement and may progress rapidly to become a serious medical condition. OHSS is characterized by a dramatic increase in vascular permeability, which can result in a rapid accumulation of fluid in the peritoneal cavity, thorax, and potentially, the pericardium. The early warning signs of OHSS developing are severe pelvic pain, nausea, vomiting, and weight gain. Abdominal pain, abdominal distension, gastrointestinal symptoms including nausea, vomiting and diarrhea, severe ovarian enlargement, weight gain, dyspnea, and oliguria have been reported with OHSS. Clinical evaluation may reveal hypovolemia, hemoconcentration, electrolyte imbalances, ascites, hemoperitoneum, pleural effusions, hydrothorax, acute pulmonary distress, and thromboembolic reactions [see *Warnings and Precautions (5.3)*]. Transient liver function test abnormalities suggestive of hepatic dysfunction with or without morphologic changes on liver biopsy have also been reported in association with OHSS.

OHSS occurs after gonadotropin treatment has been discontinued, and it can develop rapidly, reaching its maximum about seven to ten days following treatment. Usually, OHSS resolves spontaneously with the onset of menses. If there is a risk for OHSS evident prior to hCG administration [see *Warnings and Precautions (5.1)*], the hCG must be withheld. Cases of OHSS are more common, more severe, and more protracted if pregnancy occurs; therefore, women should be assessed for the development of OHSS for at least two weeks after hCG administration.

If serious OHSS occurs, gonadotropins, including hCG, should be stopped and consideration should be given as to whether the patient needs to be hospitalized. Treatment is primarily symptomatic and overall should consist of bed rest, fluid and electrolyte management, and analgesics (if needed). Because the use of diuretics can accentuate the diminished intravascular volume, diuretics should be avoided except in the late phase of resolution as described below. The management of OHSS may be divided into three phases as follows:

▪ Acute Phase:

Management should be directed at preventing hemoconcentration due to loss of intravascular volume to the third space and minimizing the risk of thromboembolic phenomena and kidney damage. Fluid intake and output, weight, hematocrit, serum and urinary electrolytes, urine specific gravity, BUN and creatinine, total proteins with albumin: globulin ratio, coagulation studies, electrocardiogram to monitor for hyperkalemia, and abdominal girth should be thoroughly assessed daily or more often based on the clinical need. Treatment, consisting of limited intravenous fluids, electrolytes, and human serum albumin is intended to normalize electrolytes while maintaining an acceptable but somewhat reduced intravascular volume. Full correction of the intravascular volume deficit may lead to an unacceptable increase in the amount of third space fluid accumulation.

▪ Chronic Phase:

After the acute phase is successfully managed as above, excessive fluid accumulation in the third space should be limited by instituting severe potassium, sodium, and fluid restriction.

▪ Resolution Phase:

As third space fluid returns to the intravascular compartment, a fall in hematocrit and increasing urinary output are observed in the absence of any increase in intake. Peripheral and/or pulmonary edema may result if the kidneys are unable to excrete third space fluid as rapidly as it is mobilized. Diuretics may be indicated during the resolution phase, if necessary, to combat pulmonary edema.

OHSS increases the risk of injury to the ovary. The ascitic, pleural, and pericardial fluid should not be removed unless there is the necessity to relieve symptoms such as pulmonary distress or cardiac tamponade. Pelvic examination may cause rupture of an ovarian cyst, which may result in hemoperitoneum, and should therefore be avoided. If bleeding occurs and requires surgical intervention, the clinical objective should be to control the bleeding and retain as much ovarian tissue as possible.

During clinical trials with Follistim or Follistim AQ Cartridge therapy, OHSS occurred in 7.6% of 105 women (OI) and 6.4% of 751 women (IVF or ICSI) treated with Follistim and Follistim AQ Cartridge, respectively.

5.3 Pulmonary and Vascular Complications

Serious pulmonary conditions (e.g., atelectasis, acute respiratory distress syndrome) have been reported in women treated with gonadotropins. In addition, thromboembolic reactions both in association with, and separate from OHSS have been reported following gonadotropin therapy. Intravascular thrombosis, which may originate in venous or arterial vessels, can result in reduced blood flow to vital organs or the extremities. Women with generally recognized risk factors for thrombosis, such as a personal or family history, severe obesity, or thrombophilia, may have an increased risk of venous or arterial thromboembolic events, during or following treatment with gonadotropins. Sequelae of such reactions have included venous thrombophlebitis, pulmonary embolism, pulmonary infarction, cerebral vascular occlusion (stroke), and arterial occlusion resulting in loss of limb and rarely in myocardial infarction. In rare cases, pulmonary complications and/or thromboembolic reactions have resulted in death. In women with recognized risk factors, the benefits of ovulation induction, in vitro fertilization (IVF) or intracytoplasmic sperm injection (ICSI) treatment need to be weighed against the risks. It should be noted, that pregnancy itself also carries an increased risk of thrombosis.

5.4 Ovarian Torsion

Ovarian torsion has been reported after treatment with Follistim AQ Cartridge and after intervention with other gonadotropins. This may be related to OHSS, pregnancy, previous abdominal surgery, past history of ovarian torsion, previous or current ovarian cyst and polycystic ovaries. Damage to the ovary due to reduced blood supply can be limited by early diagnosis and immediate detorsion.

5.5 Multi-fetal Gestation and Birth

Multi-fetal gestation and births have been reported with all gonadotropin treatments including Follistim AQ Cartridge treatment. The woman and her partner should be advised of the potential risk of multi-fetal gestation and births before starting treatment.

5.6 Congenital Anomalies

The incidence of congenital malformations after IVF or ICSI may be slightly higher than after spontaneous conception. This slightly higher incidence is thought to be related to differences in parental characteristics (e.g., maternal age, sperm characteristics) and to the higher incidence of

multi-fetal gestations after IVF or ICSI. There are no indications that the use of gonadotropins during IVF or ICSI is associated with an increased risk of congenital malformations.

5.7 Ectopic Pregnancy

Since infertile women undergoing IVF or ICSI often have tubal abnormalities, the incidence of ectopic pregnancies might be increased. Early confirmation of an intrauterine pregnancy should be determined by β -hCG testing and transvaginal ultrasound.

5.8 Spontaneous Abortion

The risk of spontaneous abortions (miscarriage) is increased with gonadotropin products. However, causality has not been established. The increased risk may be a factor of the underlying infertility.

5.9 Ovarian Neoplasms

There have been infrequent reports of ovarian neoplasms, both benign and malignant, in women who have undergone multiple drug regimens for controlled ovarian stimulation; however, a causal relationship has not been established.

5.10 Laboratory Tests

For Women:

In most instances, treatment with Follistim AQ Cartridge will result only in follicular growth and maturation. In order to complete the final phase of follicular maturation and to induce ovulation, hCG must be given following the administration of Follistim AQ Cartridge or when clinical assessment indicates that sufficient follicular maturation has occurred. The degree of follicular maturation and the timing of hCG administration can both be determined with the use of sonographic visualization of the ovaries and endometrial lining in conjunction with measurement of serum estradiol levels. The combination of transvaginal ultrasonography and measurement of serum estradiol levels is also useful for minimizing the risk of OHSS and multi-fetal gestations.

The clinical confirmation of ovulation is obtained by the following direct or indirect indices of progesterone production as well as sonographic evidence of ovulation.

Direct or indirect indices of progesterone production are:

- Urinary or serum luteinizing hormone (LH) rise
- A rise in basal body temperature
- Increase in serum progesterone
- Menstruation following the shift in basal body temperature

The following provide sonographic evidence of ovulation:

- Collapsed follicle
- Fluid in the cul-de-sac
- Features consistent with corpus luteum formation

Sonographic evaluation of the early pregnancy is also important to rule out ectopic pregnancy.

For Men:

Clinical monitoring for spermatogenesis utilizes the following indirect or direct measures:

- Serum testosterone level
- Semen analysis

5.11 Follistim Pen

The Follistim Pen is intended only for use with Follistim AQ Cartridge. The Follistim Pen is not recommended for the blind or visually impaired without the assistance of an individual with good vision who is trained in the proper use of the injection device.

6 ADVERSE REACTIONS

The following serious adverse reactions are discussed elsewhere in the labeling:

- Ovarian Hyperstimulation Syndrome [see *Warnings and Precautions* (5.2)]
- Atelectasis [see *Warnings and Precautions* (5.3)]
- Thromboembolism [see *Warnings and Precautions* (5.3)]
- Ovarian Torsion [see *Warnings and Precautions* (5.4)]
- Multi-fetal Gestation and Birth [see *Warnings and Precautions* (5.5)]
- Congenital Anomalies [see *Warnings and Precautions* (5.6)]
- Ectopic Pregnancy [see *Warnings and Precautions* (5.7)]
- Spontaneous Abortion [see *Warnings and Precautions* (5.8)]

6.1 Clinical Study Experience

Because clinical trials are conducted under widely varying conditions, adverse reactions rates observed in the clinical trials of a drug cannot be directly compared to rates in the clinical trial of another drug and may not reflect the rates observed in practice.

Ovulation Induction

In a single cycle, multi-center, assessor-blind, parallel group, comparative study, a total of 172 chronic anovulatory women who had failed to ovulate and/or conceive with clomiphene citrate therapy, were randomized and treated with Follistim (105) or a urofollitropin comparator. Adverse reactions with an incidence of greater than 2% in either treatment group are listed in Table 2.

Table 2: Common Adverse Reactions Reported at a Frequency of $\geq 2\%$ in an Assessor-Blind, Comparative Study of Anovulatory Women Receiving Ovulation Induction

System Organ Class/Adverse Reactions	Treatment Number (%) of Women	
	Follistim N=105 n (%)	Comparator N=67 n (%)
Gastrointestinal disorders		
Abdominal discomfort	3 (2.9)	1 (1.5)
Abdominal pain	3 (2.9)	2 (3.0)
Abdominal pain lower	3 (2.9)	1 (1.5)
Reproductive system and breast disorders		
Ovarian cyst	3 (2.9)	2 (3.0)
Ovarian hyperstimulation syndrome	8 (7.6)	3 (4.5)
General disorders and administration site conditions		
Pyrexia	0 (0.0)	2 (3.0)

Adverse reactions reported commonly (greater than or equal to 2% of women treated with Follistim) in other ovulation induction clinical trials were headache, abdominal distension, constipation, diarrhea, nausea, pelvic pain, uterine enlargement, vaginal hemorrhage and injection site reaction.

In Vitro Fertilization/Intracytoplasmic Sperm Injection

In a single cycle, multi-center, double-blind, parallel group, comparative study, a total of 1509 women were randomized to receive controlled ovarian stimulation with either Follistim AQ Cartridge (751 women were treated with Follistim AQ Cartridge) or a comparator and pituitary suppression with a gonadotropin releasing hormone (GnRH) antagonist as part of an in vitro fertilization (IVF) or intracytoplasmic sperm injection (ICSI) cycle. Table 3 lists adverse reactions with an incidence of greater than 2% in the group of women treated with Follistim AQ Cartridge.

Table 3: Common Adverse Reactions Reported at a Frequency of $\geq 2\%$ in a Randomized, Double-blind, Active-controlled, Comparative Study of Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization or Intracytoplasmic Sperm Injection Cycle

System Organ Class/Adverse Reactions	Follistim AQ Cartridge Treatment N = 751 n ^a (%)
Nervous System disorders	
Headache	55 (7.3%)
Gastrointestinal disorders	
Nausea	29 (3.9%)
Reproductive system and breast disorders	
Ovarian Hyperstimulation Syndrome	48 (6.4%)
Pelvic discomfort	62 (8.3%)
Pelvic Pain	41 (5.5%)
General disorders and Administration site conditions	
Fatigue	17 (2.3%)

^a n = number of women with the adverse reaction

Induction of Spermatogenesis

In an open-label, non-comparative clinical trial, 49 men with hypogonadotropic hypogonadism were enrolled to receive pretreatment with hCG, followed by combination therapy with hCG and Follistim for induction of spermatogenesis. Of the 49 men, 30 received weekly Follistim doses of 450 international units; 24 of these 30 men received a total of 48 weeks of treatment with Follistim. Adverse reactions occurring with an incidence of greater than 2% in the 30 men treated with Follistim are listed in Table 4.

Table 4: Common Adverse Reactions Reported at a Frequency of $\geq 2\%$ in an Open-Label Clinical Trial in Men with Hypogonadotropic Hypogonadism

System Organ Class/Adverse Reactions	Follistim Treatment N=30 n (%)
Nervous system disorders	
Headache	2 (6.7)
General disorders and administration site disorders	
Injection site reaction	2 (6.7)
Injection site pain	2 (6.7)
Skin and cutaneous tissue disorders	
Acne	2 (6.7)
Rash	1 (3.3)
Reproductive system and breast disorders	
Gynecomastia	1 (3.3)
Neoplasms benign, malignant and unspecified	
Dermoid cyst	1 (3.3)

6.2 Postmarketing Experience

The following adverse reactions have been identified during post approval use of Follistim and/or Follistim AQ Cartridge. Because these reactions are reported voluntarily from a population of uncertain size, it is not always possible to reliably estimate their frequency or establish a causal relationship to drug exposure.

Gastrointestinal disorders

Abdominal distension, abdominal pain, constipation, diarrhea

General disorders and administration site conditions

Injection site reaction

Reproductive system and breast disorders

Breast tenderness, metrorrhagia, ovarian enlargement, vaginal hemorrhage

Skin and subcutaneous tissue disorders

Rash

Vascular disorders

Thromboembolism [see Warnings and Precautions (5.3)]

7 DRUG INTERACTIONS

No drug-drug interaction studies have been performed.

8 USE IN SPECIFIC POPULATIONS

8.1 Pregnancy

Pregnancy Category X: Follistim AQ Cartridge should not be used during pregnancy [see Contraindications (4)].

8.3 Nursing Mothers

It is not known whether this drug is excreted in human milk. Because many drugs are excreted in human milk and because of the potential for serious adverse reactions in the nursing infant from Follistim AQ Cartridge, a decision should be made whether to discontinue nursing or to discontinue the drug, taking into account the importance of the drug to the mother.

8.4 Pediatric Use

Safety and effectiveness in pediatric patients have not been established.

8.5 Geriatric Use

Clinical studies of Follistim did not include subjects aged 65 and over.

10 OVERDOSAGE

Aside from the possibility of Ovarian Hyperstimulation Syndrome [see Warnings and Precautions (5.2, 5.3)] and multiple gestations [see Warnings and Precautions (5.5)], there is no additional information concerning the consequences of acute overdosage with Follistim AQ Cartridge.

11 DESCRIPTION

Follistim AQ Cartridge contains human follicle-stimulating hormone (hFSH), a glycoprotein hormone which is manufactured by recombinant DNA (rDNA) technology. The active drug substance, follitropin beta, has a dimeric structure containing two glycoprotein subunits (alpha and beta). Both the 92 amino acid alpha-chain and the 111 amino acid beta-chain have complex heterogeneous structures arising from two N-linked oligosaccharide chains. Follitropin beta is synthesized in a Chinese hamster ovary (CHO) cell line that has been transfected with a plasmid containing the two subunit DNA sequences encoding for hFSH. The purification process results in a highly purified preparation with a consistent hFSH isoform profile and high specific activity [as determined by the Ph. Eur. test for FSH *in vivo* bioactivity and on the basis of the molar extinction coefficient at 277 nm ($\epsilon_{277} \cdot \text{mg}^{-1} \cdot \text{cm}^{-1}$) = 1.066].

The biological activity is determined by measuring the increase in ovary weight in female rats. The intrinsic luteinizing hormone (LH) activity in follitropin beta is less than 1 international unit per 40,000 international units FSH. The compound is considered to contain no LH activity.

The amino acid sequence and tertiary structure of the product are indistinguishable from that of hFSH of urinary source. Also, based on available data derived from physico-chemical tests and bioassay, follitropin beta and follitropin alfa, another recombinant follicle-stimulating hormone product, are indistinguishable.

Follistim AQ Cartridge is a ready for use, prefilled with solution, disposable cartridge containing either 175 IU of follitropin beta in 0.210 mL (833 IU/mL), 350 IU in 0.420 mL (833 IU/mL), 650 IU in 0.780 mL (833 IU/mL) or 975 IU in 1.170 mL (833 IU/mL) of aqueous solution for multiple dose use, with a maximal deliverable dose of either 150 IU, 300 IU, 600 IU or 900 IU, respectively. Inactive ingredients in the cartridges include: benzyl alcohol NF 10 mg/mL; L-methionine USP 0.5 mg/mL; polysorbate 20 NF 0.2 mg/mL; sodium citrate (dihydrate) USP 14.7 mg/mL; sucrose NF 50 mg/mL; and water for injection USP. Hydrochloric acid NF and/or sodium hydroxide NF are used to adjust the pH to 7.

Follistim AQ Cartridge is for use only with the Follistim Pen, which features an adjustable dosing system for administering the drug in a microvolume of solution. The Follistim Pen with Follistim AQ Cartridge is intended for SUBCUTANEOUS USE ONLY. The recombinant protein in Follistim AQ Cartridge has been standardized for FSH *in vivo* bioactivity in terms of the WHO International Standard for Follicle Stimulating Hormone (FSH) Recombinant, Human for Bioassay (code 92/642), issued by the World Health Organization Expert Committee on Biological Standardization (1995). Under current storage conditions, Follistim AQ may contain up to 11% of oxidized follitropin beta.

In clinical trials with Follistim, serum antibodies to FSH or anti-CHO cell derived proteins were not detected in any of the treated patients after exposure to Follistim for up to three cycles.

12 CLINICAL PHARMACOLOGY

12.1 Mechanism of Action

Women:

Follicle-stimulating hormone (FSH), the active component in Follistim AQ Cartridge, is required for normal follicular growth, maturation, and gonadal steroid production.

In women, the level of FSH is critical for the onset and duration of follicular development, and consequently for the timing and number of follicles reaching maturity. Follistim AQ Cartridge stimulates ovarian follicular growth in women who do not have primary ovarian failure. In order to effect the final phase of follicle maturation, resumption of meiosis and rupture of the follicle in the absence of an endogenous LH surge, human chorionic gonadotropin (hCG) must be given following treatment with Follistim AQ Cartridge when patient monitoring indicates appropriate follicular development parameters have been reached.

Men:

Follistim when administered with hCG stimulates spermatogenesis in men with hypogonadotropic hypogonadism. FSH, the active component of Follistim, is the pituitary hormone responsible for spermatogenesis.

12.3 Pharmacokinetics

Pharmacokinetic parameters for Follistim AQ Cartridge were evaluated in an open-label, single-center, randomized study in 20 healthy women. Serum FSH values from a single subcutaneous injection of reconstituted Follistim lyophilized powder administered by conventional syringe were compared to those values following a single subcutaneous injection of Follistim AQ Cartridge administered with the Follistim Pen injector. Administration of follitropin beta with the Follistim Pen resulted an 18% increase in $AUC_{0-\infty}$ and C_{max} . The 18% difference in serum FSH concentrations resulting from administration of the two formulations was due to differences between the anticipated and actual volume delivered with the conventional syringe. The pharmacokinetic parameters for Follistim AQ Cartridge are as follows:

Table 5: Mean (SD) Pharmacokinetic Parameters of a Single Subcutaneous Injection of 150 IU of Follistim AQ Cartridge (n=20)

	$AUC_{0-\infty}$ (IU/L*h)	C_{max} (IU/L)	t_{max} (h)	$t_{1/2}$ (h)	CL_{app} (L/h/kg)
Follistim AQ Cartridge	215.1 (45.8)	3.4 (0.7)	12.9 (6.2)	33.4 (4.2)	0.01 (0.003)

$AUC_{0-\infty}$ Area under the curve
 C_{max} Maximum concentration
 t_{max} Time to maximum concentration
 $t_{1/2}$ Elimination half-life
 CL_{app} Clearance

Absorption:

Women:

The bioavailability of Follistim following subcutaneous and intramuscular administration was investigated in healthy, pituitary-suppressed women given a single 300 international units dose. In these women, the area under the curve (AUC), expressed as the mean \pm SD, was equivalent between the subcutaneous (455.6 ± 141.4 IU*h/L) and intramuscular (445.7 ± 135.7 IU*h/L) routes of administration. However, equivalence could not be established with respect to the peak serum FSH levels (C_{max}). The C_{max} achieved after subcutaneous administration and intramuscular administration was 5.41 ± 0.72 international units/L and 6.86 ± 2.90 international units/L, respectively. After subcutaneous or intramuscular injection the apparent dose absorbed was 77.8% and 76.4%, respectively.

The pharmacokinetics and pharmacodynamics of a single, intramuscular dose (300 international units) of Follistim were also investigated in a group (n=8) of gonadotropin-deficient, but otherwise healthy women. In these women, FSH (mean \pm SD) AUC was 339 ± 105 international units*h/L, C_{max} was 4.3 ± 1.7 international units/L. C_{max} occurred at approximately 27 ± 5.4 hours after intramuscular administration.

A multiple dose, dose proportionality, pharmacokinetic study of Follistim was completed in healthy, pituitary-suppressed, female subjects given subcutaneous doses of 75, 150, or 225 international units for 7 days. Steady-state blood concentrations of FSH were reached with all doses after 5 days of treatment based on the trough concentrations of FSH just prior to dosing (C_{trough}). Peak blood concentrations with the 75, 150, and 225 international units dose were 4.30 ± 0.60 international units/L, 8.51 ± 1.16 international units/L and 13.92 ± 1.81 international units/L, respectively.

Men:

No PK studies were conducted using Follistim AQ Cartridge in men. Exposures of follitropin beta from Follistim AQ Cartridge and Follistim are expected to be equivalent after adjusting for the 18% difference in dose [see *Dosage and Administration (2)*].

Serum levels of FSH were measured in a clinical study that compared the effects of two different dosing schedules of Follistim (150 international units three times a week or 225 international units twice a week) administered by subcutaneous injection concurrently with chorionic gonadotropin for induction of spermatogenesis in hypogonadotropic hypogonadal men. Administration of Follistim was started at Week 17. Mean serum trough concentrations of FSH remained fairly constant over the treatment period. At the end of treatment (Week 64), the mean serum trough concentrations of FSH were 2.09 international units/L in the 150 international units group and 3.22 international units/L in the 225 international units group. Serum trough concentrations of FSH measured prior to the first Follistim injection on the Mondays of active treatment period (Weeks 17 to 64) and one week after the end of treatment period are presented in Figure 1.

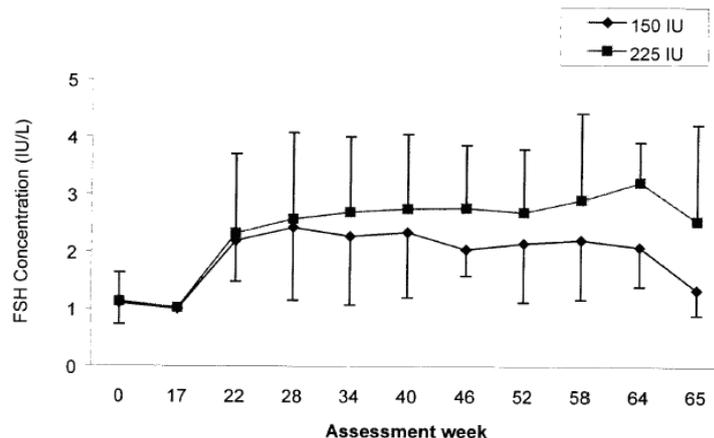


Figure 1: Mean (SD) Serum Trough Concentrations of FSH in Men Following Subcutaneous Administration of Follistim Using Two Different Dosing Schedules (150 International Units Three Times a Week or 225 International Units Twice a Week)

Distribution:

The volume of distribution of Follistim in healthy, pituitary-suppressed, women following intravenous administration of a 300 international units dose was approximately 8 L.

Metabolism:

The recombinant FSH in Follistim AQ Cartridge is biochemically very similar to urinary FSH and it is therefore anticipated that it is metabolized in the same manner.

Elimination:

The elimination half-life ($t_{1/2}$) following a single subcutaneous injection of 150 IU of Follistim AQ Cartridge in women was 33.4 (4.2) hours. The clearance was 0.01 (0.003) L/h/kg.

Use in Specific Populations:

Body weight: The effect of body weight on the pharmacokinetics of Follistim was evaluated in a group of European and Japanese women who were significantly different in terms of body weight. The European women had a body weight of (mean \pm SD) 67.4 \pm 13.5 kg and the Japanese subjects were 46.8 \pm 11.6 kg. Following a single intramuscular dose of 300 international units of Follistim, the AUC was significantly smaller in European women (339 \pm 105 international units \cdot h/L) than in Japanese women (544 \pm 201 international units \cdot h/L). However, clearance per kg of body weight was essentially the same for the respective groups (0.014 and 0.013 L/hr/kg).

Geriatric Use: The pharmacokinetics of Follistim has not been studied in geriatric subjects.

Pediatric Use: The pharmacokinetics of Follistim has not been studied in pediatric subjects.

Renal Impairment: The effect of renal impairment on the pharmacokinetics of Follistim has not been studied.

Hepatic Impairment: The effect of hepatic impairment on the pharmacokinetics of Follistim has not been studied.

13 NONCLINICAL TOXICOLOGY

13.1 Carcinogenesis, Mutagenesis, Impairment of Fertility

Long-term toxicity studies in animals have not been performed with Follistim to evaluate the carcinogenic potential of the drug. Follistim was not mutagenic in the Ames test using *S. typhimurium* and *E. coli* tester strains and did not produce chromosomal aberrations in an in vitro assay using human lymphocytes.

14 CLINICAL STUDIES

14.1 Ovulation Induction

The efficacy of Follistim for ovulation induction was evaluated in a randomized, assessor-blind, parallel-group comparative, multicenter safety and efficacy study of 172 chronic anovulatory women (105 subjects on Follistim) who had previously failed to ovulate and/or conceive during clomiphene citrate treatment. The study results for ovulation rates are summarized in Table 6 and those for pregnancy rates are summarized in Table 7.

Table 6: Cumulative Ovulation Rates

Cycle	Follistim (n=105)
First treatment cycle	72%
Second treatment cycle	82%
Third treatment cycle	85%

Table 7: Cumulative Ongoing^{*,†} Pregnancy Rates

Cycle	Follistim (n=105)
First treatment cycle	14%
Second treatment cycle	19%
Third treatment cycle	23%

* All ongoing pregnancies were confirmed after at least 12 weeks after the hCG injection.

† Study was not powered to demonstrate this outcome.

14.2 Controlled Ovarian Stimulation as Part of an In Vitro Fertilization (IVF) or Intracytoplasmic Sperm Injection (ICSI) Cycle

The efficacy of Follistim AQ Cartridge was evaluated in a randomized, double-blind, active-controlled study of 1,509 healthy normal ovulatory women (mean age, body weight, and body mass index of 32 years, 68 kg and 25 kg/m², respectively) treated for one cycle with controlled ovarian stimulation and pituitary suppression with a GnRH antagonist as part of an in vitro fertilization or intracytoplasmic sperm injection cycle. This 2008 study was conducted in Europe and North America (United States and Canada). Approximately 54% of the subjects were from North America. The overall results, as well as the results from North America only, for clinical pregnancy are summarized in Table 8.

Table 8: Pregnancy Results from Treatment With Follistim AQ Cartridge and a GnRH Antagonist in Normal Ovulatory Women Undergoing Controlled Ovarian Stimulation as Part of an In Vitro Fertilization or Intracytoplasmic Sperm Injection Cycle.* Intent-to-Treat Population (ITT)

Parameter	Follistim AQ Cartridge Overall data (n=750)	Follistim AQ Cartridge North American data (n=403)
Clinical pregnancy rate/cycle initiation [†]	41.1%	48.9%

* Single treatment cycle results

† Clinical pregnancy was assessed ≥6 weeks after transfer of one or two embryos.

14.3 Induction of Spermatogenesis

The safety and efficacy of Follistim administered by subcutaneous injection concomitantly with chorionic gonadotropin for injection (hCG) has been examined in a multicenter, open-label, non-comparator clinical study for induction of spermatogenesis in hypogonadotropic hypogonadal men. The study compared the effects of two different Follistim dosing schedules on semen parameters and serum levels of follicle stimulating hormone (FSH). The multicenter study involved a 16-week pretreatment phase with hCG at a dosage of 1,500 international units twice a week to normalize serum testosterone levels. If serum testosterone levels did not normalize after 8 weeks of hCG treatment, the hCG dose could have been increased to 3,000 international units twice a week. This phase was followed by a 48-week treatment phase. Men who were still azoospermic after the pretreatment phase were randomized to receive either 225 international units Follistim together with 1,500 international units hCG twice a week or 150 international units Follistim three times a week together with 1,500 international units hCG twice weekly. Men who required 3,000 international units of hCG twice a week in the pretreatment phase were continued on that dosage during the treatment phase. The mean age of patients in both treatment groups was approximately 30 years (range 18 to 47 years). At baseline, mean left and right testis volumes were 4.61 ± 2.94 mL and 4.57 ± 3.00 mL, respectively, in the group receiving three weekly injections of Follistim. For the group receiving two weekly injections of Follistim, the mean left and right testis volumes were 6.54 ± 2.45 mL and 7.21 ± 2.94 mL, respectively, at baseline. The primary efficacy endpoint was the percentage of patients with a mean sperm density of ≥1 x 10⁶/mL on their last two treatment assessments. The outcomes of treatment in the 30 men enrolled in the treatment phase are summarized in Table 9.

Table 9: Number of Men Receiving Follistim Who Achieved a Mean Sperm Density of ≥10⁶/mL on Their Last Two Treatment Assessments

	Follistim 150 international units three times a week (n=15)		Follistim 225 international units twice a week (n=15)		Overall (n=30)	
	n	%	n	%	n	%
Sperm Density of ≥10⁶/mL						
Yes	6	40	7	47	13	43
No	9	60	8	53	17	57

Overall, the median time to reach a sperm concentration of 10⁶ per mL was 165 days (range 25 to 327 days) in patients who demonstrated a sperm concentration of at least 10⁶ per mL. The median time to reach a sperm concentration of at least 10⁶ per mL was 186 days (range 25 to 327 days) for the 150 international units group and 141 days (range 43 to 204 days) for the 225 international units group. No pregnancy data were collected during the trial.

The local tolerance data were comparable between the two treatment groups. The mean percentage of days without pain calculated for all subjects in the treatment period was 91.3% for patients in the 150 international units (three times a week) and 76.0% for patients in the 225 international units (two times a week) Follistim treatment groups. In the 225 international units (twice per week) group, local symptoms judged as severe by the investigator were: itching in 1 patient (7%), pain in 2 patients (13%), bruising in 2 patients (13%), swelling in 2 patients (13%), and redness in 1 patient (7%). In the 150 international units (three times per week) group, 1 event in 1 patient (bruising, 7%) was judged as severe. No patient discontinued treatment due to injection site reaction or injection site pain.

16 HOW SUPPLIED/STORAGE AND HANDLING

Follistim AQ Cartridge is supplied in a box containing disposable, 29 gauge, ultra-fine, 1/2-inch, sterile BD Micro-Fine™ Pen Needles (for use with Follistim Pen available separately) packaged with one disposable prefilled 1.5 mL colorless glass cartridge, with grey rubber piston and an aluminum crimp-cap with black rubber inlay and in the following presentations:

- NDC 0052-0303-01 Follistim AQ Cartridge 175 international units per 0.210 mL (delivering 150 international units) with orange crimp-caps and 3 BD Micro-Fine Pen Needles
- NDC 0052-0313-01 Follistim AQ Cartridge 350 international units per 0.420 mL (delivering 300 international units) with silver crimp-caps and 5 BD Micro-Fine Pen Needles
- NDC 0052-0316-01 Follistim AQ Cartridge 650 international units per 0.780 mL (delivering 600 international units) with gold crimp-caps and 7 BD Micro-Fine Pen Needles
- NDC 0052-0326-01 Follistim AQ Cartridge 975 international units per 1.170 mL (delivering 900 international units) with blue crimp-caps and 10 BD Micro-Fine Pen Needles

Store refrigerated 2°-8°C (36°-46°F) until dispensed. Upon dispensing, the product may be stored by the patient at 2°-8°C (36°-46°F) until the expiration date, or at 25°C (77°F) for 3 months or until expiration date, whichever occurs first. Once the rubber inlay of the Follistim AQ Cartridge has been pierced by a needle, the product can only be stored for a maximum of 28 days at 2°-25°C (36°-77°F). Protect from light. Do not freeze.

17 PATIENT COUNSELING INFORMATION

“See FDA-Approved Patient Labeling (Patient Information)”

17.1 Dosing and Use of Follistim AQ Cartridge with Pen

Instruct women and men on the correct usage and dosing of Follistim AQ Cartridge in conjunction with the Follistim Pen. Make sure that individuals who have used other gonadotropin products delivered by a syringe are aware of differences arising from use of the pen. Women and men should read and follow all instructions in the Follistim Pen “Instructions for Use” Manual prior to administration of Follistim AQ Cartridge.

Advise women and men of the number of doses which can be extracted from the full unused Follistim AQ Cartridge that you have prescribed.

17.2 Therapy Duration and Necessary Monitoring in Women and Men Undergoing Treatment

Prior to beginning therapy with Follistim AQ Cartridge, inform women and men about the time commitment and monitoring procedures necessary to undergo treatment [see *Dosage and Administration (2)*, *Warnings and Precautions (5.10)*].

17.3 Instructions on a Missed Dose

Inform women and men that if they miss or forget to take a dose of Follistim AQ Cartridge, the next dose should not be doubled and they should call the healthcare provider for further dosing instructions.

17.4 Ovarian Hyperstimulation Syndrome

Inform women regarding the risks with use of Follistim AQ Cartridge of Ovarian Hyperstimulation Syndrome [see *Warnings and Precautions (5.2)*] and associated symptoms including lung and blood vessel problems [see *Warnings and Precautions (5.3)*] and ovarian torsion [see *Warnings and Precautions (5.4)*].

17.5 Multi-fetal Gestation and Birth

Inform women regarding the risk of multi-fetal gestations with the use of Follistim AQ Cartridge [see *Warnings and Precautions (5.5)*].

Manufactured for: Merck Sharp & Dohme Corp., a subsidiary of
 **MERCK & CO., INC.**, Whitehouse Station, NJ 08889, USA

Manufactured by: Vetter Pharma-Fertigung GmbH & Co. KG, Ravensburg, Germany

BD, BD Logo and BD Micro-Fine are trademarks of Becton, Dickinson and Company

For patent information: www.merck.com/product/patent/home.html

Copyright © 2004-2020 Merck Sharp & Dohme B.V., a subsidiary of **Merck & Co., Inc.**
All rights reserved.

uspi-mk8328-SOi-2006r014

PATIENT INFORMATION

Follistim® (Fol'-lis-tim) AQ Cartridge (follitropin beta injection)

Read the Patient Information that comes with Follistim® AQ Cartridge before you start using it and each time you get a refill. There may be new information. This information does not take the place of talking with your healthcare provider about your medical condition or treatment.

What is Follistim AQ Cartridge?

Follistim AQ is a prescription medicine that contains follicle-stimulating hormone (FSH). The medicine is taken with the Follistim Pen®.

Follistim AQ Cartridge is used:

In women:

- to help healthy ovaries to develop (mature) and release eggs
- as part of treatment programs that use special techniques (skills) to help women get pregnant by causing their ovaries to produce more mature eggs

In men:

- to help bring about the production and development of sperm

Who should not take Follistim AQ Cartridge?

Do not take Follistim AQ Cartridge if you are a Woman or Man who:

- is allergic to recombinant human FSH products
- has a high level of FSH in your blood indicating that your ovaries (women only) or testes (men only) may be permanently damaged and do not work at all
- has uncontrolled thyroid, pituitary, or adrenal gland problems
- is allergic to streptomycin or neomycin (types of antibiotics)
- has a tumor of the hypothalamus, pituitary gland, breast, uterus (women only), ovary (women only), or testis (men only)

Do not take Follistim AQ Cartridge if you are a Woman who:

- is pregnant or think you may be pregnant
- has heavy or irregular vaginal bleeding and the cause is not known
- has ovarian cysts or enlarged ovaries, not due to polycystic ovary syndrome (PCOS)

Talk to your healthcare provider before taking this medicine if you have any of the conditions listed above.

What should I tell my healthcare provider before taking Follistim AQ Cartridge?

Before you take Follistim AQ, tell your healthcare provider if you:

- have an increased risk of blood clots (thrombosis)
- have ever had a blood clot (thrombosis), or anyone in your immediate family has ever had a blood clot (thrombosis)
- had stomach (abdominal) surgery
- had twisting of your ovary (ovarian torsion)
- had or have a cyst in your ovary
- have polycystic ovary disease
- have any other medical conditions
- are breastfeeding or plan to breastfeed. It is not known if the medicine in Follistim AQ Cartridge passes into your breast milk. You and your healthcare provider should decide if you will take Follistim AQ Cartridge or breastfeed. You should not do both.

Tell your healthcare provider about all the medicines you take, including prescription and non-prescription medicines, vitamins, and herbal supplements.

Know the medicines you take. Keep a list of them and show your healthcare provider and pharmacist when you get a new medicine.

How should I use Follistim AQ Cartridge?

- Be sure that you read, understand, and follow the "Patient Instructions for Use" that come with Follistim AQ Cartridge.
- Use Follistim AQ Cartridge exactly as your healthcare provider tells you to.
- Your healthcare provider will tell you how much Follistim AQ Cartridge to use, how to inject it, and how often it should be injected.
- Do not inject Follistim AQ Cartridge at home until your healthcare provider has taught you the right way to put the cartridge and pen device together and to inject yourself.
- Do not mix any other medicines into the cartridge.
- Do not change your dose of Follistim AQ Cartridge unless your healthcare provider tells you to.
- Call your healthcare provider immediately if you use too much Follistim AQ Cartridge.
- If you miss or forget to take a dose, do not double your next dose. Ask your healthcare provider for instructions.
- Use Follistim AQ Cartridge only with the Follistim Pen.
- Do not use the Follistim Pen if you are blind or visually impaired unless you have assistance from an individual with good vision who is trained in the right way to use the pen.
- Do not re-use the BD Micro-Fine™ Pen Needle.
- Your healthcare provider will do blood and urine hormone tests while you are taking Follistim AQ Cartridge. Make sure you follow-up with your healthcare provider to have your blood and urine tested when told to do so.

Women:

- Your healthcare provider may do ultrasound scans of your ovaries. Make sure you follow-up with your healthcare provider to have your ultrasound scans.

Men:

- Your healthcare provider may test your semen while you are taking Follistim AQ Cartridge. Make sure you follow-up with your healthcare provider to give a semen sample for testing.

What are the possible side effects of Follistim AQ Cartridge?**Follistim AQ Cartridge may cause serious side effects.****Serious side effects in women include:**

- Ovarian enlargement
- Ovarian hyperstimulation syndrome (OHSS). OHSS is a serious medical problem that can happen when the ovaries are over stimulated. In rare cases it has caused death. OHSS causes fluid to build up suddenly in your stomach and chest areas and can cause blood clots to form. Call your healthcare provider right away if you have:
 - pain in your lower stomach area
 - nausea
 - vomiting
 - weight gain
 - diarrhea
 - decreased urine output
 - trouble breathing
- Lung problems. Follistim AQ Cartridge can cause you to have fluid in your lungs (atelectasis) and trouble breathing (acute respiratory distress syndrome).
- Blood clots. Follistim AQ Cartridge may increase your chance of having blood clots in your blood vessels. Blood clots can cause:
 - blood vessel problems (thrombophlebitis)
 - stroke
 - loss of your arm or leg
 - blood clot in your lungs (pulmonary embolus)
 - heart attack
- Ovarian torsion. Follistim AQ Cartridge may increase the chance of twisting of the ovaries in women with certain conditions such as OHSS, pregnancy and previous abdominal surgery. Twisting of the ovary could cause the blood flow to the ovary to be cut off.
- Pregnancy and birth of multiple babies. Having a pregnancy with more than one baby at a time increases the health risk for you and your babies. Discuss your chances of multiple births with your healthcare provider.
- Birth defects. A woman's age, certain sperm problems, genetic background of both parents and a pregnancy with multiple babies can increase the chance that your baby might have birth defects.
- Ectopic pregnancy (pregnancy outside of the womb). The chance of a pregnancy outside of the womb is increased in women with damaged fallopian tubes.
- Miscarriage. The chance of loss of an early pregnancy may be increased in women who have difficulty with becoming pregnant at all.

The most common side effects of Follistim AQ Cartridge include:**In women:**

- headache
- nausea
- stomach pain
- discomfort or pain in the lower stomach area
- cyst (closed sac) in the ovary
- feeling tired

In men:

- headache
- pain at the injection site
- bruising, swelling or redness at the injection site
- breast enlargement
- acne

These are not all the possible side effects of Follistim AQ Cartridge. For more information, ask your healthcare provider or pharmacist.

Call your healthcare provider immediately if you get worsening or strong pain in the lower stomach area (abdomen). Also, call your healthcare provider immediately if this happens some days after the last injection has been given.

Tell your healthcare provider if you have any side effect that bothers you or that does not go away.

Call your doctor for medical advice about side effects. You may report side effects to FDA at 1-800-FDA-1088.

How should I store Follistim AQ Cartridge?

- Store Follistim AQ Cartridge in the refrigerator between 2°-8°C (36°-46°F) until the expiration date.
- Follistim AQ can be stored at or below 25°C (77°F) for 3 months or until the expiration date, whichever comes first. Once the rubber inlay of the Follistim AQ Cartridge has been pierced by a needle, the product may be stored only for a maximum of 28 days at 2°-25°C (36°-77°F).
- Keep Follistim AQ Cartridge away from light.

- Do not freeze.

Keep Follistim AQ Cartridge and all medicines out of the reach of children.

General information about Follistim AQ Cartridge

Medicines are sometimes prescribed for purposes other than those listed in the Patient Information leaflet. Do not use Follistim AQ for a condition for which it was not prescribed. Do not give Follistim AQ Cartridge to other people, even if they have the same condition that you have. It may harm them.

This Patient Information leaflet summarizes the most important information about Follistim AQ Cartridge. If you would like more information, talk with your healthcare provider. You can ask your pharmacist or healthcare provider for more information about Follistim AQ Cartridge that is written for healthcare professionals.

For more information, go to www.follistim.com or call 1-866-836-5633.

What are the ingredients in Follistim AQ Cartridge?

Active ingredient: follitropin beta

Inactive ingredients: sucrose, sodium citrate, benzyl alcohol NF-10 mg/mL, L-methionine, polysorbate 20, water for injection, hydrochloric acid, and/or sodium hydroxide.

 Manufactured for: Merck Sharp & Dohme Corp., a subsidiary of
MERCK & CO., INC., Whitehouse Station, NJ 08889, USA

Manufactured by: Vetter Pharma-Fertigung GmbH & Co. KG, Ravensburg, Germany

BD, BD Logo and BD Micro-Fine are trademarks of Becton, Dickinson and Company.

For patent information: www.merck.com/product/patent/home.html

Copyright © 2004-2020 Merck Sharp & Dohme B.V., a subsidiary of **Merck & Co., Inc.**

All rights reserved.

Revised: 06/2020

usppi-mk8328-SOI-2006r015

PATIENT INSTRUCTIONS FOR USE

Follistim® (Fol'-lis-tim) AQ Cartridge (follitropin beta injection)

Read the Patient Instructions for Use that comes with Follistim® AQ Cartridge before you start using it and each time you get a refill. There may be new information. This information does not take the place of talking with your healthcare provider about your medical condition or treatment.

A. Getting Ready

- Follistim Pen is not recommended for the blind or visually impaired user without the assistance of an individual with good vision, trained in the proper use of the injection device.
- Learn about all of the parts of the Follistim Pen (See Figure 1), Follistim AQ Cartridge (See Figure 2) and the BD Micro-Fine™ Pen Needle (See Figure 3). You will need to recognize these parts to follow the directions.

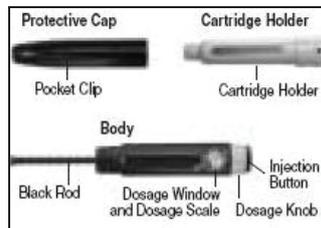


Figure 1. Follistim Pen and its Parts




Figure 2. Parts of Follistim AQ Cartridge

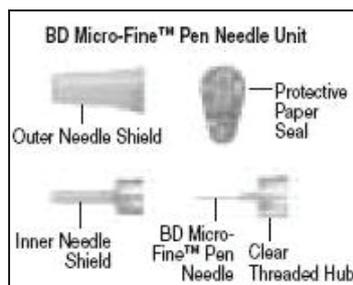


Figure 3. Parts of BD Micro-Fine Pen Needle Unit

- Remove the Cartridge out of the refrigerator.
- Injecting cold drug is likely to cause discomfort. Therefore, it is recommended you allow the drug to reach room temperature before taking the injection.
- Check the liquid in the cartridge. It should appear clear and colorless. If the solution is not clear and colorless or has particles in it, **do not use it**.
- **Gather the supplies you will need for your injection. You will need:**
 - a clean dry surface
 - alcohol
 - cotton balls or alcohol pads
 - sterile gauze
 - a puncture-proof container to throw away the used syringe and needle
- Wash your hands with soap and water and dry them before you use Follistim Pen or when you replace the cartridge.

B. Loading the Follistim Pen with the Follistim AQ Cartridge

- Holding the Pen Body firmly with one hand, pull off the Protective Cap with your other hand (See Figure 4). Put the cap aside on a clean, dry surface.



Figure 4

- Unscrew the entire Pen Body from the Cartridge Holder (See Figure 5). Place the Cartridge Holder and the Pen Body aside on a clean, dry surface.

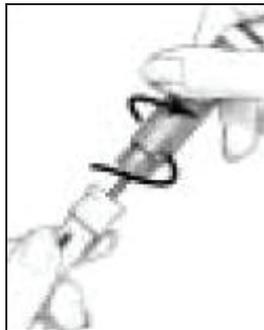


Figure 5

- Take the Follistim AQ Cartridge out of its package. Clean the rubber inlay on the cartridge with an alcohol pad. Pick up the Cartridge Holder. Put the Cartridge into the Cartridge Holder (See Figure 6). The metal rimmed cap goes in first.

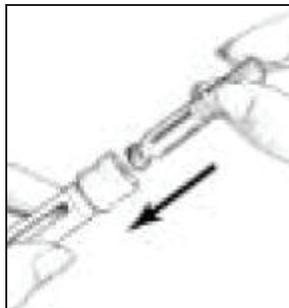


Figure 6

- Pick up the Pen Body and lower it into the Cartridge Holder. The black rod must press against the Rubber Piston on the cartridge. Screw the Pen Body fully onto the Cartridge Holder (See Figure 7). Make sure there is no gap between the Pen Body and the Cartridge Holder. The arrow (▲) on the Cartridge Holder should point to the middle of the yellow alignment mark (■) on the blue Pen Body.



Figure 7

- Clean the open end of the Cartridge Holder with an alcohol pad (See Figure 8).




Figure 8

- Pick up a new BD Micro-Fine Pen Needle that is in its Outer Needle Shield. Peel off the protective paper seal (See Figure 9). Do **not** touch the needle. Do not place the open needle on any surface. **Use Only the BD Micro-Fine 0.33 mm × 12.7 mm (29G) Pen Needles as supplied with the Follistim AQ Cartridge.**
- You must use a new BD Micro-Fine Pen Needle with each injection. Never reuse a needle. Attach a new BD Micro-Fine Pen Needle after you make sure there is a Follistim AQ Cartridge in the Cartridge.




Figure 9

- Hold the Outer Needle Shield firmly in one hand while holding the Cartridge Holder firmly in the other hand. Push the end of the Cartridge Holder into the Outer Needle Shield. Screw them tightly together (See Figure 10). Place your Follistim Pen with the loaded cartridge and attached needle, flat on a clean, dry surface.




Figure 10

C. Preparing the Injection Site

- Follistim AQ Cartridge can be injected directly into a layer of fat under your skin (subcutaneously).
- When giving a subcutaneous injection, follow your healthcare provider's instructions about changing the site for each injection. This will help lower your chances of having a skin reaction.
- **Do not** inject Follistim AQ Cartridge into an area that is tender, red, bruised, or hard.
- The recommended site for injecting Follistim AQ Cartridge subcutaneously is:
 - just below your belly button (navel) (See Figure 11)



Figure 11

- the upper outer area of your thigh (See Figure 12)




Figure 12

- Clean the skin with an alcohol wipe where the injection is to be made. Clean about two inches around the injection site where the needle will be inserted. Do not touch the cleaned area of skin.

D. Dialing the Dose Before You Give the Injection

- Your healthcare provider will decide on the dose of Follistim AQ Cartridge to be given. This dose may be increased or decreased as your treatment progresses depending on your individual type of treatment.
- Follistim AQ Cartridge using Follistim Pen can be administered subcutaneously (beneath the skin) in prescribed doses from 50 International Units (IU) up to 450 IU, in marked 25 IU increments. The Dosage Scale on the Pen has numbers and audible clicks to help you set the correct dose.
- Pull off the outer needle shield. Leave the Inner Needle Shield in place over the needle attached to the Pen (See Figure 13). Do not throw the Outer Needle Shield away, you will need it later when you throw the needle away.

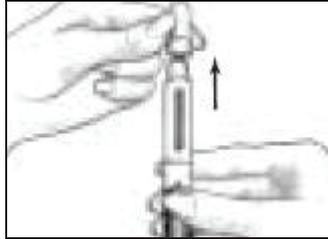


Figure 13

- Carefully remove the Inner Needle Shield and discard it (See Figure 14). Do not touch the needle or let it touch any surface while uncapped.

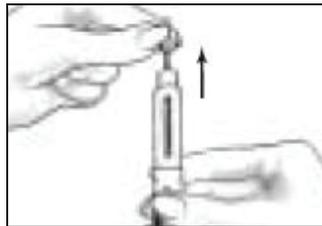


Figure 14

- Hold the Follistim Pen with the needle pointing upwards. Tap the Cartridge Holder gently with your finger to help air bubbles rise to the top of the needle. The small amount of air bubble will not affect the amount of medicine you receive.
- With a loaded new, unused cartridge:
 1. Dial the Dosage Knob until you hear one click. With the needle pointing upwards, push in the Injection Button.
 2. Look for a droplet at the tip of the needle (See Figure 15). If you see the droplet, then you can dial in your dose.
 3. If you do **not** see a droplet, repeat Step 1 (as above) until you see droplet.

You must **make sure you see a droplet** of medicine (**check the flow of medicine**) or you may **not** inject the correct amount of medicine.



Figure 15

- With a partially used cartridge, to give yourself another dose of medicine you will need to attach a new BD Micro-Fine Pen Needle and look for a droplet forming at the tip of the needle (See Figure 15 above). If you see a droplet, then you can dial in your dose.

If **no** droplet:

 1. Dial the Dosage Knob until you hear one click. With the needle pointing upwards, push in the Injection Button.
 2. Look for a droplet at the tip of the needle. If you see the droplet, then you can dial in your dose.
- Your Follistim AQ Cartridge should be one of the following:
 - Orange Metal Cap – 150 international units
 - Silver Metal Cap – 300 international units

- Gold Metal Cap – 600 international units
- Blue Metal Cap – 900 international units

If you did **not** understand that you should have one of the cartridges above, please contact your healthcare provider.

- For doses of 50 IU up to 450 IU, turn the Dosage Knob until the correct dosage aligns with the dosage markers on each side of the Dosage Window (see Figure 16).



Figure 16

- If by mistake you dial past the correct number, do not try to turn the Dosage Knob backward to fix the mistake. Continue to turn the Dosage Knob in the same direction past the 450 IU mark, as far as it will turn. The Dosage Scale must move freely. Push the Injection Button in all the way. See Figure 17. Start to dial again starting from "0" upwards. By following these directions, you will not lose any medicine from the Follistim AQ Cartridge (See "Checking the Medicine Level Remaining").



Figure 17

- If you turn the Dosage Knob backward to correct the mistake, it will not damage the Pen, but you will lose some medication from the Follistim AQ Cartridge.
- Never dial your dose or try to correct a dialing mistake when the needle is still in your skin as this may result in your receiving an incorrect dose.
- If your prescribed dose exceeds the deliverable dose of Follistim Pen or exceeds the amount remaining in the cartridge, you will need to give yourself more than one injection.

E. Giving Yourself an Injection

- Pinch a fold of skin at the cleaned injection site. **Do not** touch the cleaned area of skin.
- With the other hand hold the entire Pen with Cartridge loaded and Needle on like you would a pencil. Use a quick "dart-like" motion to insert the needle straight up and down (90-degree angle).
- Press the injection button all the way in to make sure you give yourself a full injection. (See Figure 18). Wait for five seconds before pulling the needle out of the skin. The middle of the Dosage Window should display a dot next to the "0".



Figure 18

If the injection button does **not** push in all the way, and the number in the Dosage Window does not read "0", it means there is not enough medication left in the cartridge to complete your prescribed dose. The number in the Dosage Window will give you the amount of medicine needed to complete your dose. Write this number down. This will be the number you dial for the completion of your dose. **Start over** with a new Follistim AQ Cartridge and a new needle and follow all the instructions up to this step. Make sure you choose a different injection site to complete your dose of Follistim AQ Cartridge.

- Pull out the BD Micro-Fine Needle and firmly press down on the injection site with an alcohol swab. Use the BD Micro-Fine Pen Needle for one injection only.
- Place the Outer Needle Shield on a flat table surface with the opening pointing up. The opening of the Outer Needle Shield is the wider end with the rim. Without holding on to the Outer Needle Shield, carefully insert the needle (attached to the Follistim Pen) into the opening of the Outer Needle Shield and push down firmly. The Outer Needle Shield should now be attached to the Cartridge Holder and covering the needle (See Figure 19).



Figure 19

- Grip the Outer Needle Shield and use it to unscrew the needle from the Cartridge Holder (See Figure 20). If there is Follistim AQ Cartridge medicine left for more injections, put the Pen Cap back on the Pen Body and store your Follistim Pen in a safe place in the refrigerator (not in the freezer) or at room temperature. Never store the Follistim Pen with a needle attached to it. If you are giving an injection to another person, be very careful when removing the needle from the skin. Accidental needle sticks can transmit potentially serious or grave infectious diseases.

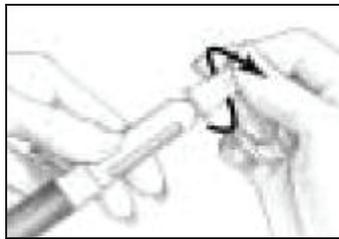


Figure 20

- Throw away the Outer Needle Shield with the used needle right away. Do not throw away in a trash can. Place it in a "special" container. (See "How Do I Throw Away Used Cartridges and Needles?")
- If there is Follistim AQ Cartridge medicine left for more injections, put the Pen Cap back on the Pen Body and store your Follistim Pen in a safe place in the refrigerator (not in the freezer) or at room temperature. Never store the Follistim Pen with a needle attached to it. If you are giving an injection to another person, be very careful when removing the needle from the skin. Accidental needle sticks can lead to serious infections.
- Unscrew the Pen Body from the Cartridge Holder with the **empty** Follistim AQ Cartridge (See Figure 21).



Figure 21

- Put the Pen Body down on a clean, dry surface and remove the empty Follistim AQ Cartridge from the Cartridge Holder (See Figure 22). Safely, dispose of the empty Follistim AQ Cartridge right away in the same "special" container that you used for the needle disposal. Do not put the cartridge in a trash can. At the end of your treatment cycle, your doctor can advise you on how to properly dispose of the container. (See "How Do I Throw Away Used Cartridges and Needles?")




Figure 22

F. Checking the Medicine Level Remaining

For women and men:

Your healthcare provider should advise you of the number of prescribed doses which can be extracted from the full unused Follistim AQ Cartridge.

- **Do not** use the cartridge beyond the advised number of doses. Otherwise, you will run the risk that there will not be enough volume of drug for your prescribed dose.

For women only:

- Keep a Follistim Pen Treatment Diary as follows:

1. Record the Follistim AQ Cartridge content on Day 1. This will either be 150, 300, 600 or 900 international units depending on what your healthcare provider has prescribed for you.
2. Record the dose you have been prescribed for your injection.
3. Subtract your Day 1 dose from the Follistim AQ Cartridge content (150, 300, 600 or 900 international units). (See example – Figure 23.) This will give you the **remaining** Follistim AQ Cartridge content after the Day 1 dose is taken.
4. Place the number determined as the content after Day 1 (see number 3) in the box as the Follistim AQ Cartridge content **available** for Day 2. (See example – Figure 23.)
5. Subtract your Day 2 dose from the Follistim AQ Cartridge content you recorded in Step 4. This will give you the **remaining** Follistim AQ Cartridge content after Day 2. Record this number of units. (See example – Figure 23.)
6. Repeat the steps to determine the Follistim AQ Cartridge content **available** and Follistim AQ Cartridge **remaining** for each day of use.

Day	Date	Dose Prescribed	Follistim AQ Cartridge Content Available	Follistim AQ Cartridge Content Remaining
1	month/day/year	150	600	450
2	month/day/year	150	450	300
3	month/day/year	150	300	150
4	month/day/year	150	150	0

Figure 23. Example of Treatment Diary Starting with a 600 International Unit Cartridge

If you do not know if there is not enough medicine left in the Follistim AQ Cartridge for your next prescribed dose, see section “If There is Not Enough Follistim AQ in the Cartridge”.

G. If There is Not Enough Follistim AQ in the Cartridge

1. If you realize **before** you inject that you do not have enough medicine remaining in your Follistim AQ Cartridge for your complete dose, follow either Option 1 or Option 2, but **not** both.
 - Option 1:
 - Dial your dose and inject the remaining content in the Follistim AQ Cartridge. The Dosage Knob Injection Button will not push in all the way (do not try to force down the button) and the Dosage Window number will not read “0” but will read the number of units you will need to complete your prescribed dose.
 - Write down the number of units needed to complete your dose.
 - Remove the needle and dispose of it properly (see “How Do I Throw Away Used Cartridges and Needles?”).
 - Using the Dosage Knob, reset the Dial Window to “0” by turning the Dosage Knob past the 450 IU mark as far as it will turn and push the Injection Button in all the way.
 - Before attempting to replace a Follistim AQ Cartridge, be sure that a BD Micro-Fine Pen Needle is not attached to the Follistim Pen.
 - Insert a new cartridge into the Follistim Pen and attach a new BD Micro-Fine needle.
 - Dial to the number of units you have written down to complete your prescribed dose.
 - Prepare a different injection site and inject the remaining drug to complete your dose (See “Giving Yourself an Injection”).
 - Option 2
 - Remove the Follistim AQ Cartridge.
 - **Start over** with a new Follistim AQ Cartridge and Insert into the Follistim Pen.
 - Follow the instructions for “Dialing the Dose” and “Giving Yourself an Injection.”
2. If you realize **after** you have inserted the needle at the injection site that you do not have enough medicine remaining in your Follistim AQ Cartridge for your complete dose:
 - Inject the remaining content in the Follistim AQ Cartridge. The Injection Button will not push in all the way and the number in the Dosage Window will not read “0” but will read the number of units you will need to complete your prescribed dose.
 - Wait 5 seconds before withdrawing the needle from your skin and gently apply pressure to the injection site with an alcohol pad.
 - Dispose of the used needle (See “How Do I Throw Away Used Cartridges and Needles?”).
 - Write down the number of units needed to complete your dose.
 - Using the Dosage Knob, reset the Dial Window to “0” by turning the Dosage Knob past the 450 IU mark as far as it will turn and push the Injection Button in all the way.

- Insert a new cartridge into the Follistim Pen and attach a new BD Micro-Fine needle.
- Dial to the number you have recorded to complete your prescribed dose.
- Prepare a different injection site and inject the remaining drug to complete your dose (See “Giving Yourself an Injection”).

H. How to Solve Problems with Follistim AQ Cartridge and Follistim Pen

If you have problems with using the Follistim AQ Cartridge and the Follistim Pen, see the following chart. If you still have problems after following the chart or if your problem is not on the chart, contact your healthcare provider.

PROBLEM	POSSIBLE CAUSES	WHAT TO DO
The Pen Body will not screw tightly into the Cartridge Holder.	Is something in the way?	Take out the Follistim Cartridge and check the Cartridge Holder to see if anything is in the way. Follow the instructions in this pamphlet to Screw the Pen Body fully onto the Cartridge Holder.
No drug is coming out while checking the flow.	The Cartridge Holder and the Pen Body are not properly screwed together.	Remove the current needle; tighten the Pen Body to the Cartridge Holder ensuring the arrow on the Cartridge Holder is pointing to the middle of the yellow alignment mark on the blue Pen Body. Attach a new needle to the Pen. Recheck the flow as follows: a. Dial the Dosage Knob until you hear one click. With needle pointing upwards, push in the Injection Button. b. Look for a droplet at the tip of the needle.
	Is the Follistim Cartridge empty?	Change to a new cartridge.
	Has the needle been properly attached to the Follistim Pen?	Remove needle and replace with a new one, ensuring that the needle is screwed on tightly to the Pen. Recheck the flow as follows: a. Dial the Dosage Knob until you hear one click. With needle pointing upwards, push in the Injection Button. b. Look for a droplet at the tip of the needle.
You are concerned that you can turn the Dosage Knob to the next number without clicking and the injection button spins freely.	This is not a problem.	The system is in the reset mode. The Injection Button and Dosage Knob must be pushed all the way down to ‘0’ to re-engage the mechanism and the correct dose can now be set. A click will be heard for each setting in the viewing window.
The Dosage Knob does not go back to ‘0’ while you are injecting.	Is the Follistim Cartridge empty?	Change to a new cartridge.
	Is the needle blocked?	a. Remove the needle from the skin and dispose of safely. b. Check the Dosage Window and note how much remaining drug to inject. c. Attach a new needle. Recheck the flow as follows: a. Dial the Dosage Knob until you hear one click. With needle pointing upwards, push in the Injection Button. b. Look for a droplet at the tip of the needle. c. Dial remaining dose.
Some of the drug is dripping out of the needle when you withdraw it from your skin.	Did you take the needle out of your skin before waiting 5 seconds as directed in Step 15?	If this happens you should inform your doctor. To avoid this problem again, you should always wait 5 seconds after you push the Injection Button before you withdraw the needle from your skin.
The needle is left on the Follistim Pen.	Have you missed any of the instructions?	Dispose of the needle in a properly secured container as instructed by your doctor. Change to a new Follistim Cartridge and a new needle.
After your last injection, a remaining volume may be left in the cartridge in addition to the normal quantity of drug dispensed.	The cartridge contains extra volume for checking the drug flow.	This is not a problem.
You cannot get the cartridge out of the Follistim Pen.	Is the needle attached?	Remove the needle from the Follistim Pen and dispose of properly. (Unscrew the Cartridge Holder from the Pen Body and take out the cartridge.)
You are not sure how much drug is left in the cartridge and you do not want to start an injection and then find out that there is not enough drug.	Have you kept good records of your doses?	In case of any doubt, you should load a new, unused Follistim Cartridge into the Follistim Pen. See “If There is Not Enough Follistim AQ in the Cartridge.” To avoid this problem again, you should record your injections. (Women should use a treatment diary.)

Important: If you have a question, always mention the Lot number of your Follistim Pen as printed on the Pen Body. If you have a complaint, please do not discard any product or packaging.

For questions on information contained in this leaflet, call 1-866-836-5633.

www.follistim.com

How Do I Throw Away Used Cartridges and Needles?

Check with your healthcare provider or pharmacist for instructions about the right way to throw away used cartridges and needles. There may be special local or state laws about how to throw away used syringes and needles.

- **Do not** throw away used cartridges and needles in the household trash and do not recycle them.
- Put used and empty cartridges and needles in a closeable, puncture-resistant container. You may use a sharps container (such as a red bio-hazard container), a hard plastic container with a screw-on cap (such as an empty detergent bottle) or in a metal container with a plastic lid, (such as a coffee can).
- When the container is full, tape around the cap or lid to make sure the cap or lid does not come off.
- When your injection is given by another person, this person must also be careful when removing the cartridge and needle and disposing of the cartridge and needle to prevent accidental needle stick injury and passing infection.

How Do I Care for the Follistim Pen?

1. Clean all exposed surfaces of the Follistim Pen with a clean, damp cloth such as a paper towel. Never wash it in water, detergent or strong medical cleaners.
2. Handle the Follistim Pen carefully to avoid causing damage. You could damage the Follistim Pen by dropping it or handling it roughly.
3. Keep the Follistim Pen away from dust and dirt.
4. Never store the Follistim Pen with a needle attached to it. If you store the Follistim Pen with the needle attached, the drug could leak out and there is risk of contamination.
5. If the Follistim Pen breaks or is damaged, do not try to fix it yourself. Contact your healthcare provider.
6. Do not share your Follistim Pen with another person.

How should I store Follistim AQ Cartridge?

- Store Follistim AQ Cartridge in the refrigerator between 2°-8°C (36°-46°F) until the expiration date.
- Follistim AQ can be stored at or below 25°C (77°F) for 3 months or until the expiration date, whichever comes first. Once the rubber inlay of the Follistim AQ Cartridge has been pierced by a needle, the product may be stored only for a maximum of 28 days at 2°-25°C (36°-77°F).
- Keep Follistim AQ Cartridge away from light.
- Do not freeze.

Keep Follistim AQ Cartridge, needles, and the disposal container, out of the reach of children.

Manufactured for: Merck Sharp & Dohme Corp., a subsidiary of
 **MERCK & CO., INC.**, Whitehouse Station, NJ 08889, USA

Manufactured by: Vetter Pharma-Fertigung GmbH & Co. KG, Ravensburg, Germany

BD, BD Logo and BD Micro-Fine are trademarks of Becton, Dickinson and Company.

For patent information: www.merck.com/product/patent/home.html

Copyright © 2004-2020 Merck Sharp & Dohme B.V., a subsidiary of **Merck & Co., Inc.**
All rights reserved.

Revised: 06/2020

usppi-mk8328-SOi-2006r015