

ellman®

Surgitron® DUAL RF™
120
4.0 MHz Radiofrequency Technology

The Technology

As pioneers of high frequency RF technology, Ellman created unparalleled surgical precision, versatility and safety. The Surgitron Dual 120 device's 4 megahertz (MHz) technology creates very little heat when cutting/coagulating tissue, resulting in minimal lateral thermal damage to surrounding tissues. The high frequency is up to eight times greater than traditional electrosurgery units, making Surgitron the ideal choice for your soft tissue cutting and coagulation needs. With over 55 years of experience, Ellman is your trusted worldwide brand for quality surgical products.

The Features

- Exceptional precision and control through two distinct frequencies – Monopolar (4.0 MHz) and Bipolar (1.7 MHz)
- 73% less thermal spread as compared to Bovie® 1250 and Valleylab® ForceFX™ in porcine tissue³
- Easy operation with clear setting display via Digital Control Panel
- Reliable, consistent energy emission through Solid State Circuitry

The Benefits


- Precision – sculpt precise incisions in very thin, delicate mobile or tension-free tissues (e.g. eyelid skin, earlobe, labia, etc.)²
- Less burning or charring of tissues¹
- Enhanced readability of histologic specimens⁸
- Excellent cosmetic results with minimal scar tissue^{4,5}
- Quick recovery⁶
- Decreased post-operative pain⁷

The Return

- With versatility across procedures, Surgitron technology is a proven workhorse that will deliver years of reliable, cost-effective performance in both hospital and office environments


HIGH FREQUENCY

How Our Technology Works




STEP 1

High frequency Radiowave energy.




STEP 2

Targeted tissue/cell readily absorbs energy due to high water content.




STEP 3

Intracellular pressure increases as water molecules expand.



STEP 4



Volatilization results in cell conversion to vapor. Process emits steam which aids in coagulation.



STEP 5

Cellular interaction enables precise dissection with tissue preservation.

4.0 MHz Minimizes Lateral Thermal Spread & Maximizes Precision

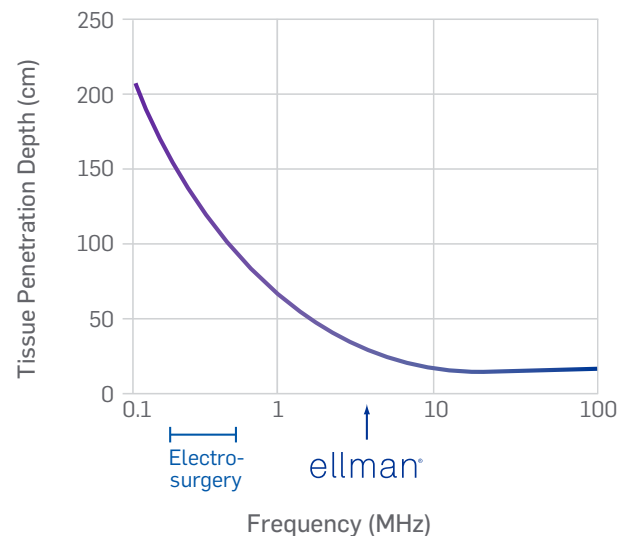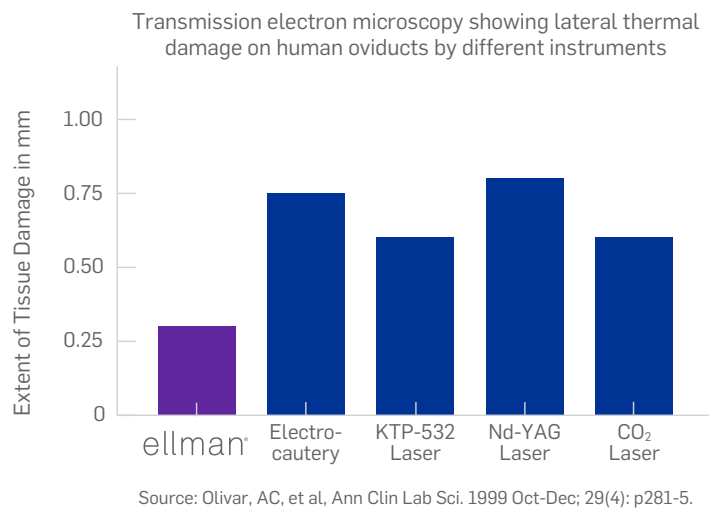


Five Distinct Waveforms for Optimal Clinical Outcomes





Cut

Micro-smooth cutting • Negligible lateral heat • Ideal for skin incision and biopsy • Best cosmetic results ^{6,7}




Blend

Cutting with hemostasis • Ideal for subcutaneous tissue dissection and planing • Especially useful in vascular areas while producing minimal amounts of lateral heat and tissue damage




Coag

Coagulation / Shrinkage • Ideal for hemostasis with controlled penetration




Fulguration

Ideal for intentional tissue destruction




Bipolar

Pinpoint, micro-coagulation • Ideal for coagulation in and around critical anatomy



Surgitron® DUAL RF™ 120

4.0 MHz Radiofrequency Technology

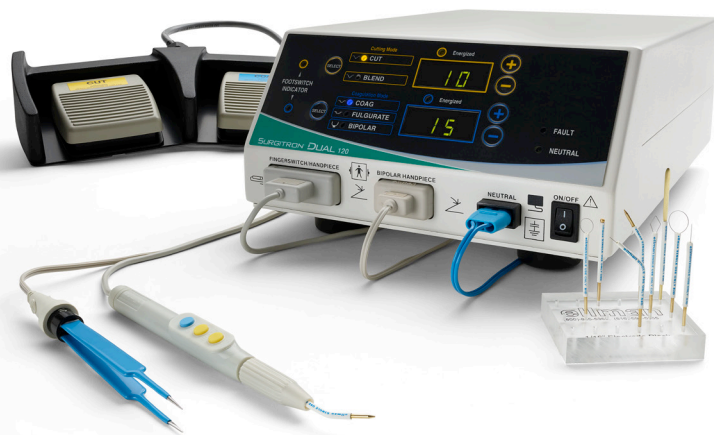

CYNOSURE
A Hologic Company

400 Karin Lane
Hicksville, NY 11801 USA

TELEPHONE 516 594 3333

TOLL FREE 800 886 2966

www.cynosure.com

	Specifications
Output Frequency	4.0MHz Monopolar 1.7MHz Bipolar
Output Power	Cut 120 W Blend 90 W Coag 60 W Fulgurate 45 W Bipolar 120 W
Electrical	100-240 VAC. 50/60 Hz
Weight	18 lbs (8.2 kg)
Dimensions	5" (12.7 cm) H x 9" (22.9 cm) W x 13" (33 cm) D

Clinical Citations

1. High frequency RF surgery minimizes burning of tissue, unlike laser or conventional electrosurgery.. Olivar, AC, et al, Ann. Clin. Lab Sci. (1999); 29 (4): p281-5.
2. Niamtu, J. Chapter 4B, "Radiowave Surgery in Oral and Maxillofacial Surgery", in Distraction Osteogenesis of the Facial Skeleton, 2007, p30-37.
3. Data on file.
4. Botero, G.E.S, J Otol Head Neck Surgery (1996); vol 24 (1), p69.
5. Aferzon, M, Derm Surgery (2002); vol 28, p735-738.
6. With less tissue destruction, healing is accelerated and patients can recover quickly. Bridenstine, J.B., Derm Surgery (1998); vol 24, p397-400.
7. High frequency RF surgery causes less trauma7. Ericsson, E, et al, The Laryngoscope (2007); vol 117, p654.
8. Minimal Heat Dissipation. Silverman, EB, et al, Veterinary Surgery (2007); vol 36, p50-56.